

Datenprotokoll

A2018037_20210721_1



Rezeptname PROGRAMM_01
 Chargennummer A2018037_20210721_1
 Ergebnis Sterilisation OK
 Startzeit 21.07.2021 - 12:55:41
 Endzeit 21.07.2021 - 16:35:57
 Dauer 03:40:16



<http://demo.geminos.eu:1111>



A2018037_20210721_1

Zeit	Nr.	Schritt	PT101 mBar	PT102 mBar	PT114 mBar	TT101 °C	F0_TT101	TT102 °C	F0_TT102	TT112 °C	F0_TT112	TT111 °C	F0_TT111	TT100 °C	TT117 °C	PT172 mBar	TT174 °C
12:55:41	1	Vorvakuum 1	4	4	10	28.3	0.0	28.2	0.0	27.5	0.0	26.9	0.0	28.5	25.1	2133	31.6
12:56:41			-455	-454	334	24.0	0.0	23.7	0.0	16.7	0.0	18.3	0.0	24.3	109.4	2149	31.5
12:57:41			-689	-685	308	22.1	0.0	22.0	0.0	18.7	0.0	18.5	0.0	22.3	108.9	2151	31.5
12:58:41			-806	-802	357	21.6	0.0	21.7	0.0	19.3	0.0	19.3	0.0	22.2	108.5	2152	31.3
12:59:41			-867	-863	301	21.7	0.0	22.1	0.0	20.0	0.0	20.0	0.0	22.8	108.0	2151	31.2
12:59:46	2	Dampf ein 1	-871	-866	297	21.7	0.0	22.2	0.0	20.0	0.0	20.0	0.0	22.8	107.7	2151	31.2
13:00:41			-742	-738	326	31.4	0.0	30.7	0.0	20.7	0.0	20.6	0.0	33.1	108.4	2149	31.1
13:01:41			-627	-624	307	43.5	0.0	42.4	0.0	21.4	0.0	21.1	0.0	46.9	108.2	2149	31.0
13:02:41			-491	-487	313	56.6	0.0	56.7	0.0	21.9	0.0	21.4	0.0	60.2	108.4	2148	30.9
13:03:41			-286	-282	300	71.5	0.0	71.2	0.0	22.2	0.0	21.7	0.0	73.6	108.3	2145	30.7
13:04:41			-76	-74	301	81.8	0.0	81.8	0.0	22.5	0.0	21.9	0.0	83.6	108.4	2139	30.6
13:05:41			200	205	301	90.8	0.0	90.8	0.0	22.6	0.0	22.1	0.0	91.9	108.4	2142	30.5
13:06:24	3	Vorvakuum 2	401	408	335	97.7	0.0	97.7	0.0	22.8	0.0	22.3	0.0	98.4	108.0	2144	30.4
13:06:41			172	178	356	101.7	0.0	101.5	0.0	89.9	0.0	90.1	0.0	101.5	108.3	2149	30.4
13:07:41			-293	-288	322	89.8	0.0	89.7	0.0	84.8	0.0	84.8	0.0	89.9	108.2	2154	30.3
13:08:41			-535	-527	356	80.0	0.0	79.9	0.0	76.0	0.0	76.0	0.0	80.0	107.6	2152	30.3
13:09:41			-658	-650	324	72.7	0.0	72.6	0.0	69.1	0.0	69.1	0.0	72.6	108.0	2152	30.2
13:10:41			-731	-722	355	67.3	0.0	67.1	0.0	64.1	0.0	64.0	0.0	67.0	107.8	2153	30.2
13:11:41			-779	-770	332	63.1	0.0	62.9	0.0	60.1	0.0	60.0	0.0	62.7	107.8	2154	30.3
13:12:41			-813	-804	347	59.7	0.0	59.4	0.0	56.9	0.0	57.0	0.0	59.1	107.6	2153	30.3
13:13:41			-839	-830	302	57.0	0.0	56.6	0.0	54.2	0.0	54.7	0.0	56.2	107.8	2152	30.4
13:14:41			-860	-851	316	54.6	0.0	54.1	0.0	52.3	0.0	52.9	0.0	53.6	108.0	2150	30.4
13:15:18	4	Dampf ein 2	-870	-861	356	53.5	0.0	52.9	0.0	51.3	0.0	53.9	0.0	52.1	107.0	2150	30.5
13:15:41			-653	-645	352	68.5	0.0	68.9	0.0	50.3	0.0	52.0	0.0	67.4	107.5	2146	30.5
13:16:41			-177	-170	302	92.7	0.0	92.8	0.0	50.4	0.0	51.1	0.0	92.3	107.2	2142	30.6
13:17:41			230	234	320	104.2	0.0	104.2	0.0	49.9	0.0	50.4	0.0	103.8	107.8	2141	30.6
13:18:05	5	Vorvakuum 3	402	407	304	108.3	0.0	108.2	0.0	49.7	0.0	50.1	0.0	108.1	106.7	2147	30.7
13:18:41			63	67	309	102.6	0.0	102.3	0.0	97.8	0.0	97.8	0.0	102.6	107.6	2152	30.7
13:19:41			-234	-227	310	93.1	0.0	93.1	0.0	90.2	0.0	90.3	0.0	93.2	107.6	2153	30.8
13:20:41			-430	-421	323	85.4	0.0	85.4	0.0	82.3	0.0	82.3	0.0	85.5	107.8	2153	31.0
13:21:41			-562	-553	301	78.8	0.0	78.8	0.0	76.1	0.0	76.1	0.0	78.8	107.0	2152	31.1
13:22:41			-657	-647	307	73.1	0.0	73.2	0.0	70.7	0.0	71.4	0.0	73.1	107.4	2152	31.2
13:23:41			-725	-714	303	68.4	0.0	68.8	0.0	67.5	0.0	71.9	0.0	68.3	107.0	2151	31.4
13:24:41			-775	-764	310	64.9	0.0	66.0	0.0	69.2	0.0	69.4	0.0	65.5	107.4	2151	31.5
13:25:41			-810	-799	316	62.6	0.0	64.5	0.0	67.2	0.0	67.1	0.0	66.2	107.8	2151	31.7
13:26:41			-837	-826	307	61.9	0.0	63.4	0.0	65.1	0.0	64.8	0.0	65.9	107.2	2153	31.8
13:27:41			-858	-846	307	61.9	0.0	62.5	0.0	63.4	0.0	62.9	0.0	65.5	107.3	2153	31.9
13:28:26	6	Dampf ein 3	-870	-858	309	62.2	0.0	62.3	0.0	62.4	0.0	62.1	0.0	65.0	107.4	2154	32.0
13:28:41			-713	-700	305	63.7	0.0	64.2	0.0	62.1	0.0	61.7	0.0	65.3	107.1	2153	32.1
13:29:41			-99	-94	307	95.2	0.0	95.2	0.0	60.5	0.0	60.2	0.0	94.7	107.2	2152	32.2
13:30:41			367	374	304	107.7	0.1	107.7	0.1	58.8	0.0	58.8	0.0	107.4	106.8	2154	32.3
13:30:47	7	Vorvakuum 4	397	405	308	108.6	0.1	108.6	0.1	58.6	0.0	58.6	0.0	108.3	106.8	2153	32.3
13:31:41			-40	-33	355	99.4	0.1	99.3	0.1	95.9	0.0	96.0	0.0	99.5	106.9	2159	32.4
13:32:41			-286	-278	316	91.2	0.1	91.1	0.1	88.4	0.0	88.5	0.0	91.2	107.8	2159	32.5
13:33:41			-461	-451	301	84.0	0.1	83.9	0.1	82.2	0.0	82.3	0.0	84.0	106.8	2156	32.6
13:34:41			-585	-575	304	77.7	0.1	77.6	0.1	80.5	0.0	80.3	0.0	77.6	107.0	2156	32.8
13:35:41			-676	-665	327	73.3	0.1	73.3	0.1	77.0	0.0	76.9	0.0	74.5	107.5	2155	33.0
13:36:41			-742	-732	311	72.2	0.1	71.2	0.1	74.0	0.0	73.8	0.0	73.5	107.4	2153	33.2
13:37:41			-790	-780	323	71.6	0.1	69.0	0.1	71.3	0.0	71.3	0.0	72.7	107.8	2153	33.4
13:38:41			-825	-815	330	70.7	0.1	67.5	0.1	69.3	0.0	69.3	0.0	71.8	106.7	2152	33.6
13:39:41			-850	-839	303	69.8	0.1	66.7	0.1	67.6	0.0	67.6	0.0	70.9	106.9	2151	33.8
13:40:41			-870	-858	311	69.1	0.1	66.5	0.1	66.0	0.0	66.0	0.0	69.5	107.6	2149	34.0
13:40:43	8	Dampf ein 4	-870	-859	308	69.1	0.1	66.5	0.1	66.0	0.0	65.9	0.0	69.5	107.3	2149	34.0
13:41:41			-224	-214	317	90.3	0.1	90.3	0.1	64.6	0.0	64.7	0.0	89.6	107.8	2147	34.2
13:42:41			257	261	301	105.1	0.1	105.1	0.1	62.9	0.0	63.3	0.0	104.8	106.8	2113	34.3
13:43:02	9	Heizen	402	407	309	108.4	0.1	108.5	0.1	62.3	0.0	62.7	0.0	108.1	106.8	2133	34.3
13:43:41			636	642	310	113.4	0.2	113.4	0.2	113.4	0.1	113.5	0.1	113.1	106.9	2144	34.4
13:44:41			950	955	305	119.0	0.5	119.0	0.5	118.7	0.4	119.0	0.4	118.8	106.8	2146	34.5
13:45:41			1245	1250	323	123.7	1.6	123.7	1.6	123.3	1.4	123.6	1.5	123.5	107.2	2145	34.6
13:46:24	10	Sterilisieren	1322	1326	327	125.0	3.1	124.9	3.1	124.4	2.8	124.6	2.9	124.8	107.3	2146	34.8

Zeit	Nr.	Schritt	PT101 mBar	PT102 mBar	PT114 mBar	TT101 °C	F0_TT101	TT102 °C	F0_TT102	TT112 °C	F0_TT112	TT111 °C	F0_TT111	TT100 °C	TT117 °C	PT172 mBar	TT174 °C
13:46:41			1331	1336	332	125.2	3.8	125.1	3.8	124.5	3.4	124.8	3.6	125.1	107.4	2147	35.0
13:47:41			1329	1333	341	125.3	6.4	125.2	6.3	124.4	5.6	124.8	5.9	125.2	107.6	2150	36.2
13:48:41			1337	1340	349	125.2	8.9	125.2	8.9	124.6	7.7	124.8	8.2	125.1	107.7	2152	37.5
13:49:41			1332	1335	358	125.3	11.5	125.2	11.4	124.5	9.9	124.8	10.6	125.2	107.9	2152	39.3
13:50:41			1340	1344	372	125.2	14.1	125.2	13.9	124.6	12.1	124.8	12.9	125.2	108.2	2153	41.4
13:51:41			1329	1332	392	125.3	16.7	125.2	16.5	124.5	14.3	124.8	15.2	125.2	108.6	2153	43.6
13:52:41			1335	1340	416	125.3	19.3	125.2	19.1	124.5	16.5	124.8	17.6	125.2	109.1	2154	46.1
13:53:41			1335	1339	443	125.3	21.9	125.2	21.6	124.5	18.7	124.8	20.0	125.2	109.7	2155	49.6
13:54:41			1335	1340	469	125.3	24.5	125.2	24.2	124.5	20.9	124.8	22.3	125.2	110.2	2157	52.1
13:55:41			1332	1337	493	125.3	27.1	125.2	26.7	124.5	23.1	124.8	24.6	125.2	110.7	2158	54.2
13:56:41			1333	1336	517	125.3	29.8	125.2	29.3	124.5	25.3	124.8	27.0	125.2	111.2	2159	57.1
13:57:41			1341	1344	539	125.3	32.3	125.2	31.8	124.6	27.5	124.8	29.3	125.2	111.6	2159	59.0
13:58:41			1338	1344	559	125.3	35.0	125.2	34.4	124.6	29.7	124.8	31.7	125.2	112.0	2158	63.5
13:59:41			1334	1337	578	125.3	37.6	125.2	37.0	124.6	31.9	124.9	34.0	125.2	112.4	2157	70.2
14:00:41			1333	1337	591	125.3	40.2	125.2	39.5	124.6	34.1	124.9	36.3	125.2	112.7	2157	70.7
14:01:41			1338	1340	603	125.3	42.8	125.2	42.1	124.6	36.3	124.9	38.7	125.2	112.9	2156	70.9
14:02:41			1327	1331	613	125.3	45.4	125.2	44.6	124.5	38.5	124.8	41.1	125.2	113.0	2094	83.7
14:03:41			1330	1333	621	125.3	48.0	125.2	47.2	124.6	40.7	124.9	43.4	125.2	113.2	2090	81.7
14:04:41			1341	1343	627	125.3	50.6	125.2	49.7	124.6	42.9	124.9	45.7	125.2	113.3	2145	80.6
14:05:41			1338	1340	632	125.3	53.3	125.2	52.3	124.5	45.1	124.8	48.1	125.2	113.4	2152	88.9
14:06:41			1329	1331	636	125.3	55.9	125.2	54.8	124.5	47.3	124.9	50.4	125.2	113.4	2152	88.7
14:07:41			1328	1332	628	125.3	58.5	125.2	57.4	124.5	49.5	124.8	52.8	125.2	113.3	2152	87.6
14:08:41			1336	1338	634	125.3	61.1	125.2	60.0	124.6	51.7	124.9	55.2	125.2	113.3	2151	94.0
14:09:41			1338	1343	641	125.3	63.7	125.2	62.5	124.6	53.8	124.9	57.5	125.2	113.4	2152	91.9
14:10:41			1334	1338	646	125.3	66.3	125.2	65.0	124.5	56.1	124.8	59.9	125.2	113.4	2152	90.8
14:11:41			1327	1329	650	125.3	68.9	125.2	67.6	124.5	58.3	124.8	62.2	125.2	113.4	2150	90.4
14:12:41			1327	1331	648	125.3	71.5	125.2	70.1	124.5	60.5	124.8	64.5	125.2	113.2	2148	93.7
14:13:41			1332	1334	652	125.3	74.2	125.2	72.7	124.6	62.7	124.9	66.9	125.2	113.1	2146	93.1
14:14:41			1327	1329	653	125.3	76.8	125.2	75.3	124.5	64.9	124.8	69.3	125.2	112.9	2145	93.7
14:15:41			1329	1331	659	125.3	79.4	125.2	77.8	124.6	67.1	124.9	71.6	125.2	112.9	2148	94.4
14:16:41			1339	1344	668	125.3	82.0	125.2	80.4	124.6	69.3	124.9	74.0	125.2	112.9	2150	93.6
14:17:41			1331	1334	674	125.3	84.6	125.2	82.9	124.6	71.5	124.9	76.3	125.2	112.9	2151	92.8
14:18:24	11	Abstr. klein	1335	1338	677	125.3	86.5	125.2	84.8	124.6	73.1	124.9	78.0	125.2	112.9	2152	92.7
14:18:41			1274	1278	677	124.7	87.2	124.6	85.4	123.8	73.6	124.1	78.6	124.7	112.9	2151	97.3
14:19:41			1078	1082	672	121.8	88.9	121.8	87.1	120.9	75.0	121.2	80.1	121.8	112.7	2148	94.1
14:20:41			900	905	657	119.1	89.7	118.9	88.0	118.1	75.7	118.4	80.8	118.9	112.4	2147	93.0
14:20:42	12	Abstr. groß	891	898	654	119.0	89.8	118.9	88.0	117.8	75.7	118.3	80.9	118.9	112.4	2147	93.4
14:21:41			419	424	606	111.1	90.0	110.5	88.2	108.6	75.8	108.8	81.0	110.7	111.4	2145	97.1
14:22:33	13	Vorvakuum 1	193	199	550	106.0	90.1	105.3	88.3	100.9	75.9	103.4	81.1	105.4	110.2	2148	94.4
14:22:41			80	84	579	104.9	90.1	103.8	88.3	92.4	75.9	91.8	81.1	104.0	109.4	2149	93.4
14:23:41			-304	-293	534	94.2	90.1	91.1	88.3	93.6	75.9	93.4	81.1	91.4	110.1	2155	91.2
14:24:41			-501	-490	490	89.5	90.1	86.3	88.3	89.0	75.9	88.8	81.1	86.2	109.0	2152	90.8
14:25:41			-635	-623	454	87.3	90.1	84.1	88.3	85.1	75.9	84.8	81.1	84.7	108.1	2149	90.6
14:26:41			-726	-713	425	85.3	90.1	83.3	88.3	81.8	75.9	81.5	81.1	83.9	107.4	2147	90.2
14:27:41			-788	-775	396	83.2	90.1	82.3	88.3	79.2	75.9	79.0	81.1	82.3	106.7	2145	89.9
14:28:41			-830	-817	366	81.8	90.1	80.5	88.3	77.1	75.9	76.9	81.1	80.3	106.0	2145	89.6
14:29:41			-860	-846	340	81.5	90.1	79.5	88.3	75.3	75.9	75.2	81.1	78.8	105.3	2146	89.2
14:30:07	14	Trocknen 1	-870	-856	331	81.2	90.1	79.4	88.3	74.6	75.9	74.5	81.1	78.4	105.0	2146	89.0
14:30:41			-882	-868	317	80.7	90.1	79.3	88.3	73.7	75.9	73.7	81.1	78.3	104.8	2146	88.8
14:31:41			-898	-884	456	80.0	90.1	79.2	88.3	72.4	75.9	72.5	81.1	78.6	110.0	2146	88.7
14:32:41			-909	-894	400	80.5	90.1	79.6	88.3	71.4	75.9	71.5	81.1	79.0	108.4	2145	87.8
14:33:41			-917	-903	358	80.9	90.1	80.2	88.3	70.4	75.9	70.6	81.1	79.5	107.3	2144	85.1
14:34:41			-922	-908	317	81.3	90.1	80.4	88.3	69.4	75.9	69.8	81.1	79.7	106.3	2143	83.7
14:35:41			-927	-913	356	81.6	90.1	80.7	88.3	68.5	75.9	68.9	81.1	79.9	108.0	2142	82.9
14:36:41			-930	-916	315	81.7	90.1	80.7	88.3	42.6	75.9	68.1	81.1	79.9	107.0	2142	82.4
14:37:41			-933	-919	329	81.7	90.1	80.6	88.3	38.7	75.9	41.4	81.1	79.7	107.4	2141	82.1
14:38:41			-935	-921	334	81.5	90.1	80.4	88.3	38.5	75.9	41.7	81.1	79.4	107.7	2138	82.0
14:39:41			-936	-923	336	81.1	90.1	80.0	88.3	40.1	75.9	45.8	81.1	78.9	107.8	2140	81.5
14:40:07	15	Dampfstoss 1	-937	-923	315	80.8	90.1	79.8	88.3	40.1	75.9	46.4	81.1	78.6	107.0	2142	81.2
14:40:41			-365	-353	335	84.4	90.1	84.3	88.3	41.2	75.9	43.8	81.1	83.4	107.7	2144	80.9
14:41:41			431	434	309	108.8	90.1	108.7	88.3	41.8	75.9	43.3	81.1	108.3	106.8	2146	80.3
14:42:26	16	Abstroemen 1	803	806	341	116.3	90.2	116.3	88.4	42.7	75.9	43.5	81.1	116.0	107.5	2143	80.1
14:42:41			718	722	352	115.9	90.3	115.8	88.5	115.0	75.9	115.3	81.1	115.8	107.8	2143	81.6
14:43:41			384	390	349	109.7	90.5	109.6	88.7	107.8	76.0	108.1	81.2	109.7	107.8	2146	80.2
14:44:26	17	Vorvakuum 2	190	193	319	105.3	90.5	105.2	88.7	97.7	76.1	103.0	81.2	105.3	107.0	2147	78.7
14:44:41			-1	3	309	101.5	90.5	101.3	88.7	90.8	76.1	90.3	81.2	101.6	106.9	2152	78.1
14:45:41			-369	-360	316	88.7	90.5	88.9	88.7	89.7	76.1	89.5	81.2	88.6	107.2	2152	75.9
14:46:41			-586	-576	329	85.0	90.5	83.5	88.7	84.8	76.1	84.6	81.2	85.0	107.6	2148	74.1
14:47:41			-727	-715	307	84.4	90.5	78.6	88.7	81.8	76.1	81.6	81.2	84.4	106.9	2145	72.4
14:48:41			-815	-803	355	83.2	90.5	76.5	88.7	80.1	76.1	79.9	81.2	83.4	108.2	2141	71.1
14:49:41			-864	-852	318	82.4	90.5	75.6	88.7	78.7	76.1	78.8	81.2	82.4	107.2	2141	70.0


Zeit	Nr.	Schritt	PT101 mBar	PT102 mBar	PT114 mBar	TT101 °C	F0_TT101	TT102 °C	F0_TT102	TT112 °C	F0_TT112	TT111 °C	F0_TT111	TT100 °C	TT117 °C	PT172 mBar	TT174 °C
14:49:52	18	Trocknen 2	-871	-858	311	82.5	90.5	75.7	88.7	78.5	76.1	78.6	81.2	82.1	107.0	2141	69.8
14:50:41			-891	-879	311	82.0	90.5	75.6	88.7	77.7	76.1	78.0	81.2	81.5	107.0	2145	69.2
14:51:41			-906	-895	303	81.9	90.5	76.2	88.7	76.7	76.1	77.2	81.2	81.3	106.8	2147	68.5
14:52:41			-916	-904	325	81.8	90.5	76.5	88.7	75.7	76.1	76.3	81.2	80.8	107.5	2148	67.9
14:53:41			-921	-910	312	81.5	90.5	76.6	88.7	74.5	76.1	75.3	81.2	80.6	107.0	2150	67.3
14:54:41			-926	-914	300	81.6	90.5	76.9	88.7	73.4	76.1	74.3	81.2	80.4	106.7	2150	66.8
14:55:41			-929	-917	317	81.3	90.5	77.0	88.7	71.6	76.1	73.1	81.2	79.8	107.2	2150	66.0
14:56:41			-931	-920	304	80.7	90.5	76.9	88.7	38.8	76.1	39.6	81.2	79.1	106.8	2148	65.1
14:57:41			-933	-921	316	80.0	90.5	76.7	88.7	38.3	76.1	43.1	81.2	78.2	107.1	2142	64.3
14:58:41			-935	-923	303	79.2	90.5	76.3	88.7	38.2	76.1	47.2	81.2	77.1	106.8	2142	63.5
14:59:41			-936	-924	317	78.4	90.5	75.9	88.7	38.3	76.1	48.5	81.2	76.0	107.2	2143	62.8
14:59:52	19	Belueften 2	-935	-921	310	78.2	90.5	75.8	88.7	38.3	76.1	49.2	81.2	75.8	106.9	1639	62.6
15:00:41			-616	-606	283	78.0	90.5	75.8	88.7	41.5	76.1	48.0	81.2	75.2	106.3	-97	62.1
15:01:41			-229	-224	249	77.0	90.5	75.1	88.7	41.9	76.1	48.7	81.2	74.7	105.5	63	61.4
15:02:41			137	142	218	76.2	90.5	74.8	88.7	42.4	76.1	48.7	81.2	75.0	104.8	342	60.8
15:03:26	20	Abstroemen 2	402	406	249	75.8	90.5	74.8	88.7	42.7	76.1	48.4	81.2	75.3	104.3	1311	60.4
15:03:41			375	378	326	75.8	90.5	74.8	88.7	46.0	76.1	50.9	81.2	75.5	108.1	2145	60.4
15:04:41			290	293	339	76.0	90.5	75.4	88.7	54.7	76.1	64.1	81.2	76.4	108.2	2164	60.2
15:05:41			216	219	309	76.0	90.5	75.7	88.7	58.9	76.1	67.4	81.2	76.7	106.9	2166	59.7
15:05:57	21	Vorvakuum 3	197	202	300	76.0	90.5	75.8	88.7	62.7	76.1	67.6	81.2	76.7	106.7	2166	59.6
15:06:41			-313	-307	330	76.1	90.5	76.1	88.7	70.9	76.1	71.0	81.2	76.2	108.0	2200	59.1
15:07:41			-648	-640	303	76.1	90.5	76.3	88.7	71.6	76.1	71.8	81.2	75.7	106.8	2162	58.5
15:08:41			-797	-788	308	76.9	90.5	77.2	88.7	71.4	76.1	71.9	81.2	75.9	106.9	2159	57.9
15:09:41			-865	-855	317	77.9	90.5	78.1	88.7	70.4	76.1	71.4	81.2	76.0	107.3	2157	57.3
15:09:49	22	Trocknen 3	-870	-860	310	78.0	90.5	78.2	88.7	70.2	76.1	71.2	81.2	76.0	107.0	2156	57.2
15:10:41			-895	-885	302	78.3	90.5	78.3	88.7	68.7	76.1	70.0	81.2	75.8	106.7	2155	56.6
15:11:41			-912	-902	311	77.4	90.5	77.3	88.7	67.1	76.1	68.6	81.2	75.2	107.0	2155	56.0
15:12:41			-923	-913	332	76.0	90.5	75.8	88.7	65.7	76.1	66.8	81.2	73.7	108.0	2155	55.4
15:13:41			-931	-920	305	74.5	90.5	74.2	88.7	64.3	76.1	65.3	81.2	71.8	106.8	2155	54.7
15:14:41			-935	-925	314	72.9	90.5	72.6	88.7	62.7	76.1	63.9	81.2	69.8	107.1	2154	54.0
15:15:41			-938	-927	340	71.3	90.5	70.9	88.7	61.0	76.1	62.4	81.2	67.9	106.7	2155	53.4
15:16:41			-940	-929	306	69.8	90.5	69.4	88.7	59.4	76.1	61.0	81.2	66.3	106.8	2155	52.7
15:17:41			-941	-930	311	68.5	90.5	68.0	88.7	58.1	76.1	59.8	81.2	64.9	107.1	2154	52.1
15:18:41			-942	-931	376	67.3	90.5	66.8	88.7	56.9	76.1	58.7	81.2	63.7	106.8	2152	51.5
15:19:41			-942	-931	305	66.3	90.5	65.7	88.7	55.7	76.1	57.7	81.2	62.7	106.8	2151	51.0
15:19:49	23	Belueften 3	-941	-929	302	66.1	90.5	65.5	88.7	55.5	76.1	57.5	81.2	62.6	106.7	645	50.9
15:20:41			-598	-588	277	66.1	90.5	65.4	88.7	53.2	76.1	56.0	81.2	62.6	106.2	-99	50.5
15:21:41			-210	-206	244	65.5	90.5	64.8	88.7	51.5	76.1	54.5	81.2	63.8	105.4	76	49.9
15:22:41			155	160	212	65.4	90.5	64.9	88.7	50.2	76.1	53.2	81.2	65.1	104.7	358	49.6
15:23:23	24	Abstroemen 3	403	405	191	65.5	90.5	65.1	88.7	49.5	76.1	52.4	81.2	66.0	104.2	568	49.3
15:23:41			301	303	318	67.4	90.5	67.2	88.7	65.5	76.1	66.9	81.2	67.5	107.8	2146	49.2
15:24:06	25	Vorvakuum 4	192	197	309	70.1	90.5	70.1	88.7	70.5	76.1	71.5	81.2	69.8	107.0	2159	49.1
15:24:41			-222	-215	306	72.6	90.5	72.6	88.7	72.6	76.1	72.5	81.2	71.9	106.9	2221	48.8
15:25:41			-608	-600	305	74.0	90.5	74.1	88.7	72.6	76.1	72.6	81.2	72.9	106.8	2164	48.5
15:26:41			-782	-772	305	75.4	90.5	75.4	88.7	72.4	76.1	72.7	81.2	73.5	106.9	2161	48.1
15:27:41			-861	-851	309	76.4	90.5	76.6	88.7	71.4	76.1	72.1	81.2	73.5	106.9	2158	47.8
15:27:53	26	Trocknen 4	-870	-860	303	76.6	90.5	76.7	88.7	71.1	76.1	71.9	81.2	73.5	106.8	2158	47.7
15:28:41			-896	-886	313	76.5	90.5	76.5	88.7	69.6	76.1	70.7	81.2	73.3	107.2	2156	47.4
15:29:41			-914	-904	325	74.6	90.5	74.4	88.7	67.8	76.1	69.0	81.2	71.9	107.9	2155	47.1
15:30:41			-926	-915	300	72.5	90.5	72.3	88.7	66.1	76.1	67.0	81.2	69.5	106.7	2154	46.8
15:31:41			-933	-923	303	70.5	90.5	70.2	88.7	64.4	76.1	65.4	81.2	67.0	106.8	2153	46.5
15:32:41			-938	-927	304	68.5	90.5	68.2	88.7	62.6	76.1	63.7	81.2	64.6	106.8	2153	46.2
15:33:41			-941	-930	307	66.7	90.5	66.3	88.7	60.8	76.1	62.1	81.2	62.6	106.9	2153	46.0
15:34:41			-942	-932	313	65.1	90.5	64.6	88.7	59.0	76.1	60.5	81.2	60.9	107.2	2153	45.7
15:35:41			-943	-933	316	63.7	90.5	63.2	88.7	57.5	76.1	59.1	81.2	59.6	107.4	2153	45.4
15:36:41			-944	-933	336	62.4	90.5	61.9	88.7	56.1	76.1	57.9	81.2	58.6	106.8	2154	45.2
15:37:41			-944	-934	304	61.3	90.5	60.7	88.7	55.0	76.1	56.7	81.2	57.6	106.8	2155	44.9
15:37:53	27	Belueften 4	-943	-931	321	61.1	90.5	60.5	88.7	54.7	76.1	56.5	81.2	57.4	107.7	1656	44.9
15:38:41			-624	-615	292	61.1	90.5	60.3	88.7	53.1	76.1	55.4	81.2	57.7	106.5	-103	44.7
15:39:41			-236	-232	263	60.7	90.5	60.0	88.7	51.7	76.1	54.1	81.2	59.1	105.9	55	44.5
15:40:41			131	134	229	60.8	90.5	60.3	88.7	50.6	76.1	53.0	81.2	60.8	105.1	338	44.3
15:41:27	28	Abstroemen 4	403	406	255	61.1	90.5	60.7	88.7	49.9	76.1	52.1	81.2	61.9	104.6	1325	44.1
15:41:41			368	371	340	61.5	90.5	61.2	88.7	57.4	76.1	58.8	81.2	62.6	108.0	2137	44.1
15:42:41			281	284	302	64.0	90.5	64.1	88.7	66.4	76.1	67.9	81.2	66.8	106.8	2159	43.9
15:43:41			215	218	304	65.5	90.5	65.8	88.7	67.1	76.1	68.6	81.2	68.7	106.8	2161	43.6
15:43:58	29	Vorvakuum 5	191	196	313	65.8	90.5	66.1	88.7	67.1	76.1	68.6	81.2	69.0	107.3	2162	43.5
15:44:41			-293	-286	305	70.8	90.5	71.4									

Zeit	Nr.	Schritt	PT101 mBar	PT102 mBar	PT114 mBar	TT101 °C	F0_TT101	TT102 °C	F0_TT102	TT112 °C	F0_TT112	TT111 °C	F0_TT111	TT100 °C	TT117 °C	PT172 mBar	TT174 °C
15:48:41			-903	-893	305	75.5	90.5	75.6	88.7	69.8	76.1	70.9	81.2	72.9	106.8	2149	42.5
15:49:41			-919	-909	305	73.1	90.5	73.1	88.7	67.8	76.1	68.9	81.2	70.5	106.9	2149	42.3
15:50:41			-929	-919	304	70.8	90.5	70.7	88.7	65.9	76.1	66.9	81.2	67.6	106.9	2146	42.2
15:51:41			-936	-926	305	68.5	90.5	68.4	88.7	64.0	76.1	65.1	81.2	64.7	106.8	2149	42.0
15:52:41			-940	-930	305	66.4	90.5	66.2	88.7	62.0	76.1	63.3	81.2	62.2	106.8	2153	41.8
15:53:41			-943	-933	303	64.5	90.5	64.2	88.7	60.0	76.1	61.5	81.2	60.1	106.8	2153	41.6
15:54:41			-944	-934	305	62.9	90.5	62.5	88.7	58.1	76.1	59.8	81.2	58.7	106.8	2152	41.5
15:55:41			-945	-935	306	61.5	90.5	61.1	88.7	56.5	76.1	58.4	81.2	57.4	106.9	2154	41.3
15:56:41			-945	-935	307	60.2	90.5	59.7	88.7	55.1	76.1	57.1	81.2	56.4	106.9	2154	41.2
15:57:41	31	Belueften 5	-942	-934	307	59.1	90.5	58.7	88.7	53.9	76.1	55.8	81.2	55.5	106.9	852	41.1
15:57:41			-934	-926	306	59.1	90.5	58.7	88.7	53.9	76.1	55.8	81.2	55.5	106.9	-70	41.1
15:58:41			-539	-531	283	59.0	90.5	58.4	88.7	52.3	76.1	54.6	81.2	56.2	106.3	-89	41.0
15:59:41			-152	-149	254	58.8	90.5	58.2	88.7	51.1	76.1	53.5	81.2	57.8	105.7	102	40.8
16:00:41			212	216	220	59.0	90.5	58.6	88.7	50.1	76.1	52.4	81.2	59.3	104.9	405	40.7
16:01:15	32	Abstroemen 5	402	405	284	59.2	90.5	58.9	88.7	49.6	76.1	51.9	81.2	60.1	104.5	1303	40.6
16:01:41			250	252	312	63.8	90.5	63.8	88.7	69.1	76.1	70.4	81.2	63.9	107.6	2152	40.6
16:01:55	33	Vorvakuum 6	199	202	302	65.7	90.5	65.8	88.7	71.0	76.1	72.1	81.2	65.5	106.8	2160	40.6
16:02:41			-314	-308	305	70.9	90.5	71.1	88.7	73.7	76.1	73.6	81.2	70.1	106.8	2205	40.4
16:03:41			-653	-647	302	73.4	90.5	73.5	88.7	73.9	76.1	73.9	81.2	71.9	106.7	2162	40.3
16:04:41			-805	-797	301	75.0	90.5	75.2	88.7	73.3	76.1	73.7	81.2	72.7	106.7	2159	40.2
16:05:38	34	Trocknen 6	-870	-861	302	75.7	90.5	76.0	88.7	72.1	76.1	72.9	81.2	72.7	106.7	2156	40.1
16:05:41			-873	-864	342	75.7	90.5	76.0	88.7	72.0	76.1	72.8	81.2	72.7	107.2	2156	40.1
16:06:41			-904	-894	300	74.5	90.5	74.7	88.7	69.9	76.1	71.1	81.2	72.0	106.7	1944	40.0
16:07:41			-920	-911	331	72.0	90.5	72.2	88.7	67.9	76.1	69.0	81.2	69.3	106.7	1924	39.9
16:08:41			-930	-921	322	69.6	90.5	69.7	88.7	66.0	76.1	67.0	81.2	66.2	107.9	1920	39.8
16:09:41			-937	-928	312	67.3	90.5	67.3	88.7	64.0	76.1	65.1	81.2	63.3	107.3	1932	39.7
16:10:41			-941	-932	312	65.1	90.5	65.1	88.7	61.9	76.1	63.2	81.2	60.7	107.5	2138	39.6
16:11:41			-943	-934	311	63.3	90.5	63.1	88.7	59.7	76.1	61.4	81.2	58.9	107.3	2163	39.6
16:12:41			-945	-935	310	61.7	90.5	61.4	88.7	57.8	76.1	59.7	81.2	57.4	107.2	2164	39.5
16:13:41			-945	-936	310	60.3	90.5	59.9	88.7	56.2	76.1	58.1	81.2	56.3	107.3	2163	39.4
16:14:41			-946	-936	310	59.0	90.5	58.7	88.7	54.8	76.1	56.8	81.2	55.3	107.3	2159	39.3
16:15:38	35	Belueften 6	-944	-936	314	58.1	90.5	57.6	88.7	53.7	76.1	55.6	81.2	54.4	107.6	1342	39.3
16:15:41			-914	-905	309	58.1	90.5	57.6	88.7	53.5	76.1	55.5	81.2	54.4	107.1	-93	39.2
16:16:41			-523	-516	287	58.0	90.5	57.3	88.7	52.2	76.1	54.4	81.2	55.3	106.4	-88	39.2
16:17:41			-136	-133	263	57.8	90.5	57.2	88.7	51.1	76.1	53.4	81.2	56.8	105.9	123	39.1
16:18:41			232	234	230	58.0	90.5	57.6	88.7	50.1	76.1	52.4	81.2	58.5	105.1	425	39.0
16:19:11	36	Abstroemen 6	401	404	214	58.3	90.5	57.9	88.7	49.7	76.1	51.8	81.2	59.1	104.7	568	39.0
16:19:41			238	240	308	63.5	90.5	63.5	88.7	69.8	76.1	71.0	81.2	63.4	107.3	1986	39.0
16:19:53	37	Vorvakuum 7	195	201	332	65.1	90.5	65.1	88.7	71.0	76.1	72.2	81.2	64.7	107.7	1893	39.0
16:20:41			-329	-323	294	70.8	90.5	70.8	88.7	74.0	76.1	73.9	81.2	69.6	106.6	1928	38.9
16:21:41			-661	-654	274	73.3	90.5	73.3	88.7	74.1	76.1	74.1	81.2	71.4	106.1	1932	38.8
16:22:41			-809	-800	248	74.7	90.5	74.9	88.7	73.4	76.1	73.8	81.2	72.0	105.5	1927	38.7
16:23:36	38	Trocknen 7	-871	-862	220	75.3	90.5	75.7	88.7	72.2	76.1	73.0	81.2	72.2	104.9	2130	38.7
16:23:41			-875	-866	217	75.3	90.5	75.7	88.7	72.0	76.1	72.9	81.2	72.2	104.8	2145	38.7
16:24:41			-905	-896	186	73.8	90.5	74.2	88.7	69.9	76.1	71.1	81.2	71.3	104.0	2167	38.6
16:25:41			-921	-911	157	71.3	90.5	71.6	88.7	67.8	76.1	68.9	81.2	68.5	103.3	2169	38.5
16:26:41			-931	-921	131	68.8	90.5	69.1	88.7	65.8	76.1	66.9	81.2	65.4	102.7	2166	38.5
16:27:41			-937	-928	108	66.5	90.5	66.6	88.7	63.8	76.1	65.0	81.2	62.4	102.2	2163	38.4
16:28:41			-941	-932	88	64.4	90.5	64.4	88.7	61.7	76.1	63.1	81.2	60.0	101.6	2158	38.4
16:29:41			-944	-934	69	62.6	90.5	62.5	88.7	59.6	76.1	61.2	81.2	58.2	101.1	2155	38.3
16:30:41			-945	-936	52	61.0	90.5	60.8	88.7	57.6	76.1	59.5	81.2	56.8	100.7	2153	38.3
16:31:41			-946	-936	38	59.6	90.5	59.3	88.7	56.0	76.1	57.9	81.2	55.7	100.3	2152	38.2
16:32:41			-946	-937	24	58.5	90.5	58.1	88.7	54.6	76.1	56.5	81.2	54.7	99.9	1968	38.2
16:33:36	39	Belueften 7	-946	-935	12	57.5	90.5	57.1	88.7	53.5	76.1	55.4	81.2	53.9	99.6	626	38.1
16:33:41			-904	-896	11	57.5	90.5	57.0	88.7	53.3	76.1	55.3	81.2	53.9	99.5	-162	38.1
16:34:41			-526	-519	5	57.3	90.5	56.7	88.7	52.0	76.1	54.1	81.2	54.7	98.2	-116	38.0
16:35:41			-157	-154	7	57.1	90.5	56.5	88.7	50.9	76.1	53.1	81.2	56.3	94.4	92	38.0
16:35:57	40	PROGRAMM ENDE	-67	-64	6	57.1	0.0	56.6	0.0	50.7	0.0	52.8	0.0	56.6	93.3	1163	38.0

Anzahl Alarme: 3

Zeit	Nr.	Alarmtext
14:46:45	991	Test Alarm 1
14:47:40	992	Test Alarm 2
14:54:29	993	Test Alarm 3

Druck [Bar]

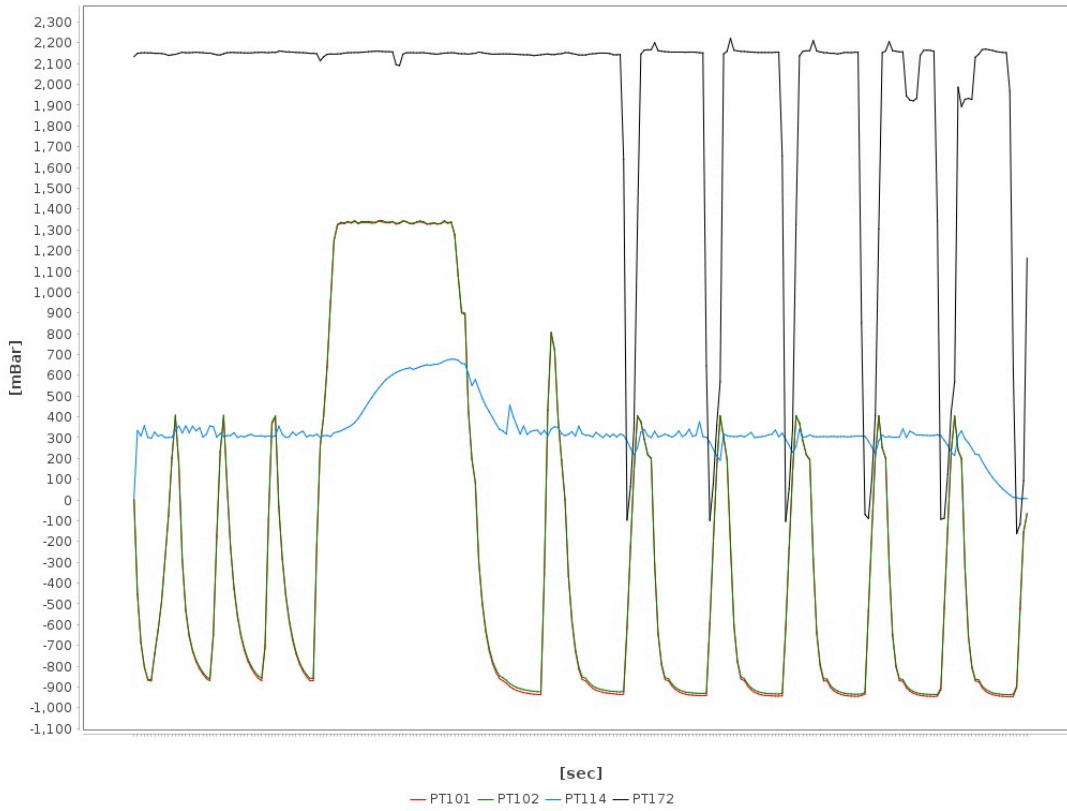

Temperatur [gradC]

